


Inspection Certification	LKT-1612		
Customer	Skywalk	Stand	Rev. 1.2 - 28.06.2013
Testlocation	Bad Grönenbach	12,5 N	Messungenauigkeit
Date	04.04.17		
Bending	5000	Temp./humi.	20,1° - 44%
Line-Manufacturer	Liros		
Articel	PPSLS-125	Line diameter	
Req. strength	1250 N		
Material	Dyneema / PES	Color	blue
length of seam - mm		Kind of seam	NZZ
Description/Norm	Bending test confirm EN 926-1 & LTF 91/09		

Results		
Max. strength unbended	1159,0 N	92,7 % from req. Strength
Max. strength Test 1	1203,0 N	96,2 %
Max. strength Test 2	1184,0 N	94,7 %
Max. strength Test 3	1150,0 N	92,0 %
Test Result average	1179,0 N	Result with MU
Test Result minimum	1150,0 N	1137,5 N

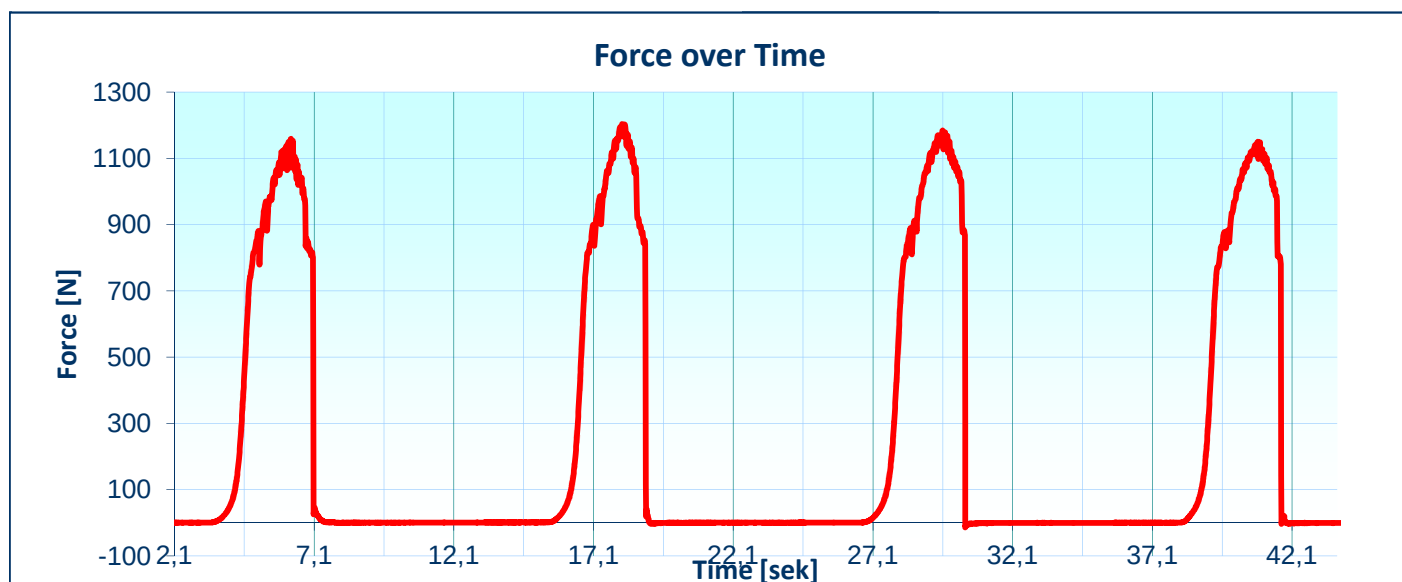

Bad Grönenbach, den 04.04.2017

Guido Reisch

Inspektor

EAPR GmbH

Test laboratory for Parachute- and Paraglidersystems